


3.7165, TiAlV4 ELI, ISO 5832-3

Implant Steel – Data Sheet US



Zapp is certified to ISO 9001

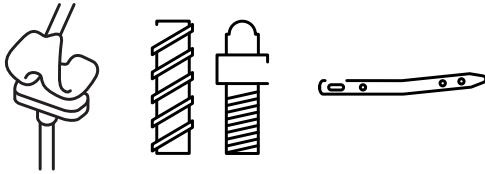

Zapp® 3.7165 ELI (TiAl6V4) – Medical Implant Steel

Zapp® 3.7165 (Extra-Low-Interstitial) is a high-strength titanium alloy with a very good strength-to-density ratio.

ELI (Extra Low Interstitial) means that the contents of the elements iron (Fe) and oxygen (O) are limited in comparison to the conventional alloy.

This supports the bone cell growth on the implant surface and accelerate their firm adhesion (osseointegration)

The material shows exceptional biocompatibility and is easily accepted by the body.

Typical Applications

- Cages and Bars for the spine area
- Permanent implants for knees and hips
- Bone screws and nails
- Dental abutments

Weldability

The TIG and MIG processes using, for example, argon with a purity of 99.999% are suitable. Other suitable welding processes are plasma, laser and electron beam welding. All semi-finished products to be welded must be dry and free from impurities and oxides.

Complete inert gas protection including the underside of the seam must be guaranteed because the high affinity of titanium to atmospheric gases can lead to oxidation / embrittlement of the surface from approx. 482 °F.

Machining

In the annealed state, Zapp® 3.7165 ELI has optimal conditions for the most effective machining.

Magnetism

Zapp® 3.7165 ELI is not magnetizable.

Corrosion Resistance

Zapp® 3.7165 shows good corrosion resistance in oxidizing media, which is due to the formation of a dense, firmly adhering oxide layer. If damaged, it quickly reforms in the presence of oxygen.

Standard Designation

- According to DIN EN TiAl6V4
- Grade 3.7165
- According to ISO 5832-3
- According to ASTM B 348, F136
- According to UNS R56401

Typical Chemical Composition (approx. values)

	C	N	O	H	Al	Fe
Min.	-	-	-	-	5.50	-
Max.	≤ 0.08	≤ 0.05	≤ 0.13	≤ 0.012	6.50	≤ 0.25
	V	Ti				
Min.	3.50					
Max.	4.50	rest				

Hot Working

Preferably in an electrically heated oven under inert gas or in a vacuum. Otherwise, the atmosphere should be adjusted to be slightly oxidizing to neutral.

Annealing: approx. 1,340 °F

Holding time: 1-4 h

Cooling: air

We always recommend consulting our technical advisors about heat treatment

Mechanical Properties*

Tensile strength R_m [ksi]	≥ 125
Yield strength $R_{p0.2}$ [ksi]	≥ 115
Elongation A [%]	≥ 10

*Example for mechanical properties < 1.75 inch

Physical Properties

Modulus of elasticity E at 68 °F [ksi]	16,534.3
Density ρ [lb/in ³]	0.161
Thermal conductivity λ at 68 °F [Btu in / hr ft ² °F]	46.46
Coefficient of thermal expansion α [μ in / in °F]	
68 – 212 °F	4.8
68 – 392 °F	5.1
68 – 572 °F	5.3
68 – 932 °F	5.6
Specific heat c at 68 °F [Btu/lb °F]	133.8
Specific electrical resistance ρ at 68 °F [Ω* ^{circular-mil} /ft]	330.8
Melting range [°F]	> 3,056
α / β Transus [°F]	~ 1,814

MEDICAL ALLOYS
Zapp Precision Metals GmbH
Letmather Straße 69
58239 Schwerte
medicalalloys@zapp.com
www.zapp.com

Further information regarding our products and locations are available in our image brochure and under www.zapp.com

The illustrations, drawings, dimensional and weight data and other information included in this data sheet are intended only for the purposes of describing our products and represent non-binding average values. They do not constitute quality data, nor can they be used as the basis for any guarantee of quality or durability. The applications presented serve only as illustrations and can be construed neither as quality data nor as a guarantee in relation to the suitability of the material. This cannot substitute for comprehensive consultation on the selection of our products and on their use in a specific application. The brochure is not subject to change control.

Last revision: June 20266